

ADJUSTMENT RECORD BPS-800




S/N: BP8-2544-XXXX

DATE: 07/11/2025

AMBIENT TEMPERATURE: 21,54°C

ADJUSTMENT DEVICE:
METEOSENSE EQB4, ABSOLUTE PRESSURE
ACCURACY ±0.02 HPA

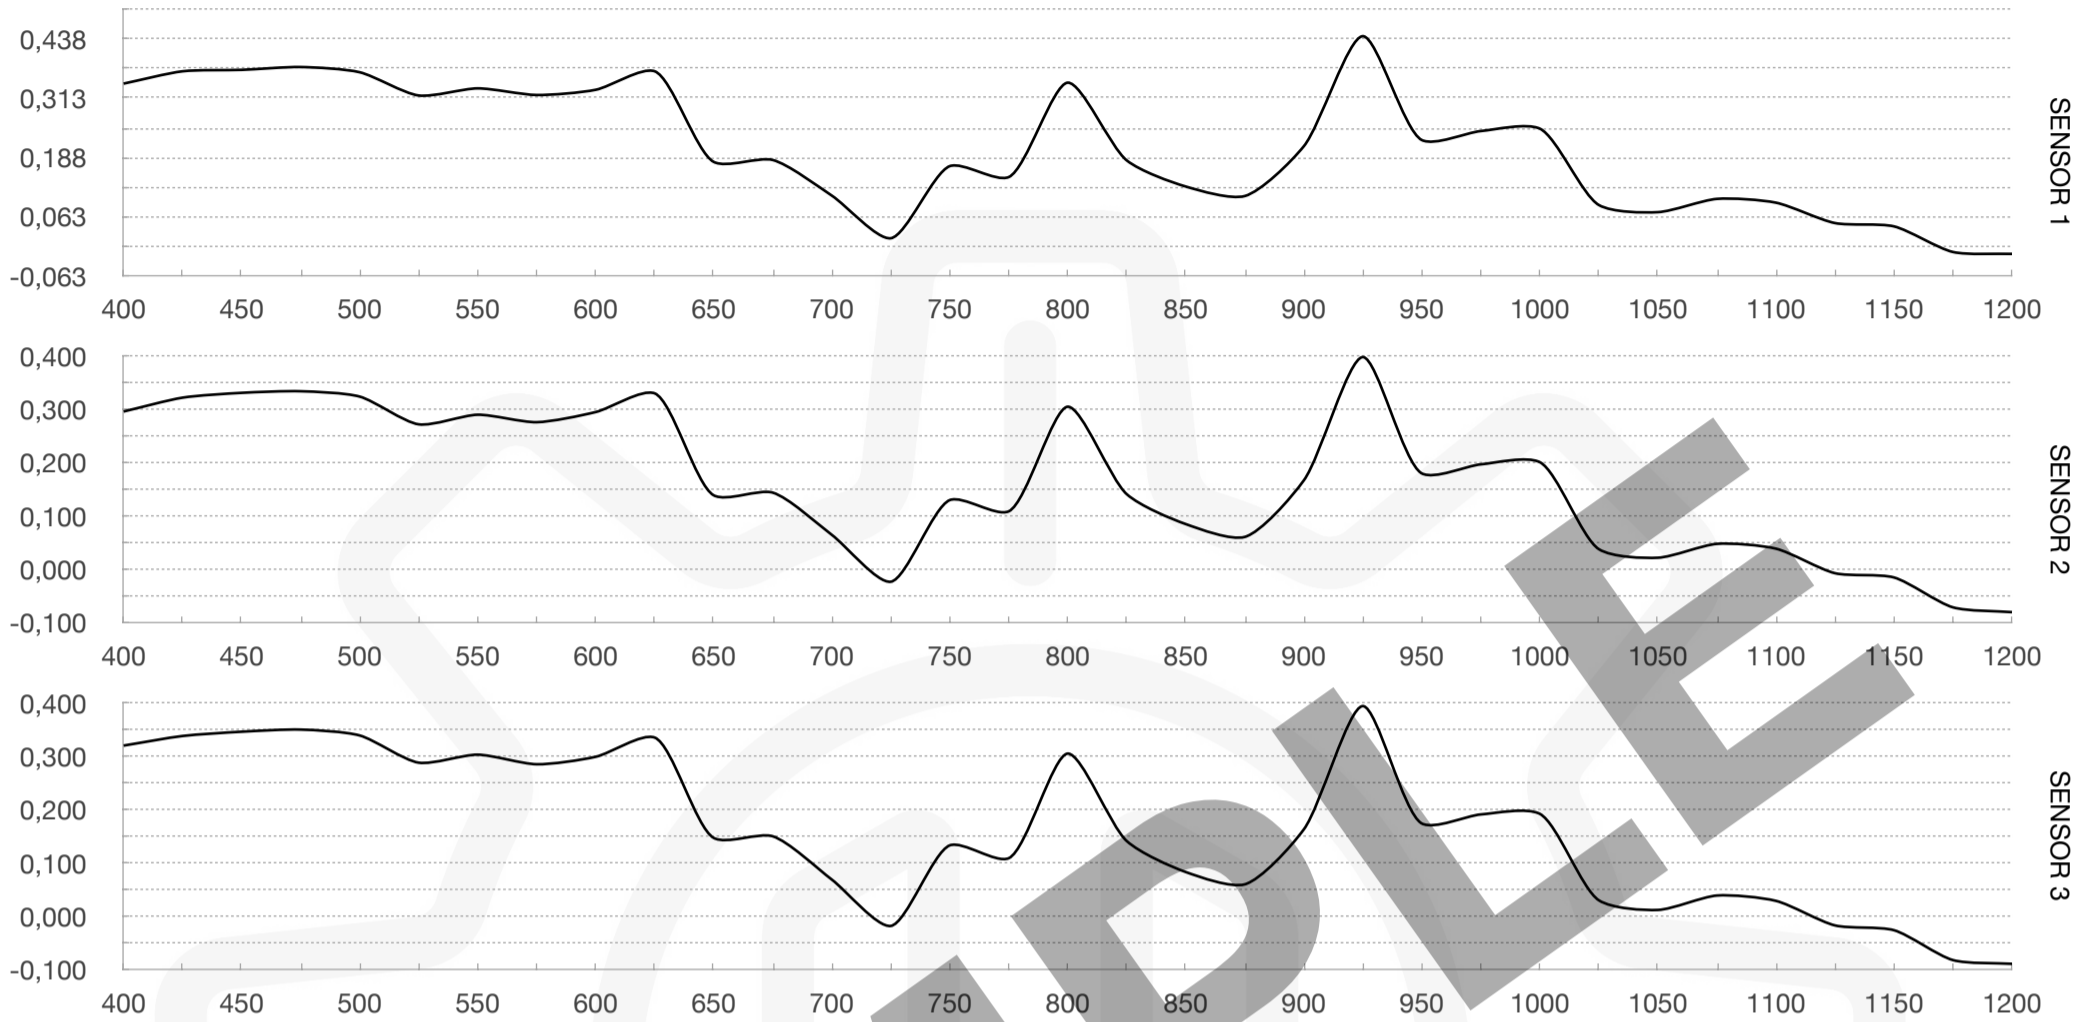

HPA	SENSOR 1 IN HPA	DEVIATION SENSOR 1	SENSOR 2 IN HPA	DEVIATION SENSOR 2	SENSOR 3 IN HPA	DEVIATION SENSOR 3
400	400,343	0,343	400,296	0,296	400,320	0,320
425	425,369	0,369	425,322	0,322	425,338	0,338
450	450,372	0,372	450,331	0,331	450,346	0,346
475	475,378	0,378	475,334	0,334	475,350	0,350
500	500,367	0,367	500,324	0,324	500,339	0,339
525	525,318	0,318	525,272	0,272	525,288	0,288
550	550,333	0,333	550,290	0,290	550,303	0,303
575	575,319	0,319	575,276	0,276	575,285	0,285
600	600,330	0,330	600,295	0,295	600,299	0,299
625	625,369	0,369	625,330	0,330	625,335	0,335
650	650,178	0,178	650,139	0,139	650,147	0,147
675	675,182	0,182	675,144	0,144	675,150	0,150
700	700,107	0,107	700,065	0,065	700,069	0,069
725	725,017	0,017	724,977	-0,023	724,982	-0,018
750	750,169	0,169	750,130	0,130	750,133	0,133
775	775,146	0,146	775,109	0,109	775,109	0,109
800	800,345	0,345	800,305	0,305	800,305	0,305
825	825,181	0,181	825,141	0,141	825,141	0,141
850	850,126	0,126	850,085	0,085	850,083	0,083
875	875,106	0,106	875,061	0,061	875,060	0,060
900	900,211	0,211	900,167	0,167	900,163	0,163
925	925,443	0,443	925,398	0,398	925,394	0,394
950	950,224	0,224	950,180	0,180	950,174	0,174
975	975,243	0,243	975,197	0,197	975,191	0,191
1000	1000,248	0,248	1000,201	0,201	1000,192	0,192
1025	1025,087	0,087	1025,038	0,038	1025,030	0,030
1050	1050,072	0,072	1050,022	0,022	1050,012	0,012
1075	1075,100	0,100	1075,048	0,048	1075,039	0,039
1100	1100,092	0,092	1100,039	0,039	1100,029	0,029
1125	1125,049	0,049	1124,993	-0,007	1124,983	-0,017
1150	1150,042	0,042	1149,985	-0,015	1149,974	-0,026
1175	1174,988	-0,012	1174,929	-0,071	1174,918	-0,082
1200	1199,984	-0,016	1199,920	-0,080	1199,911	-0,089